



1/7

BEST AVAILABLE COPY

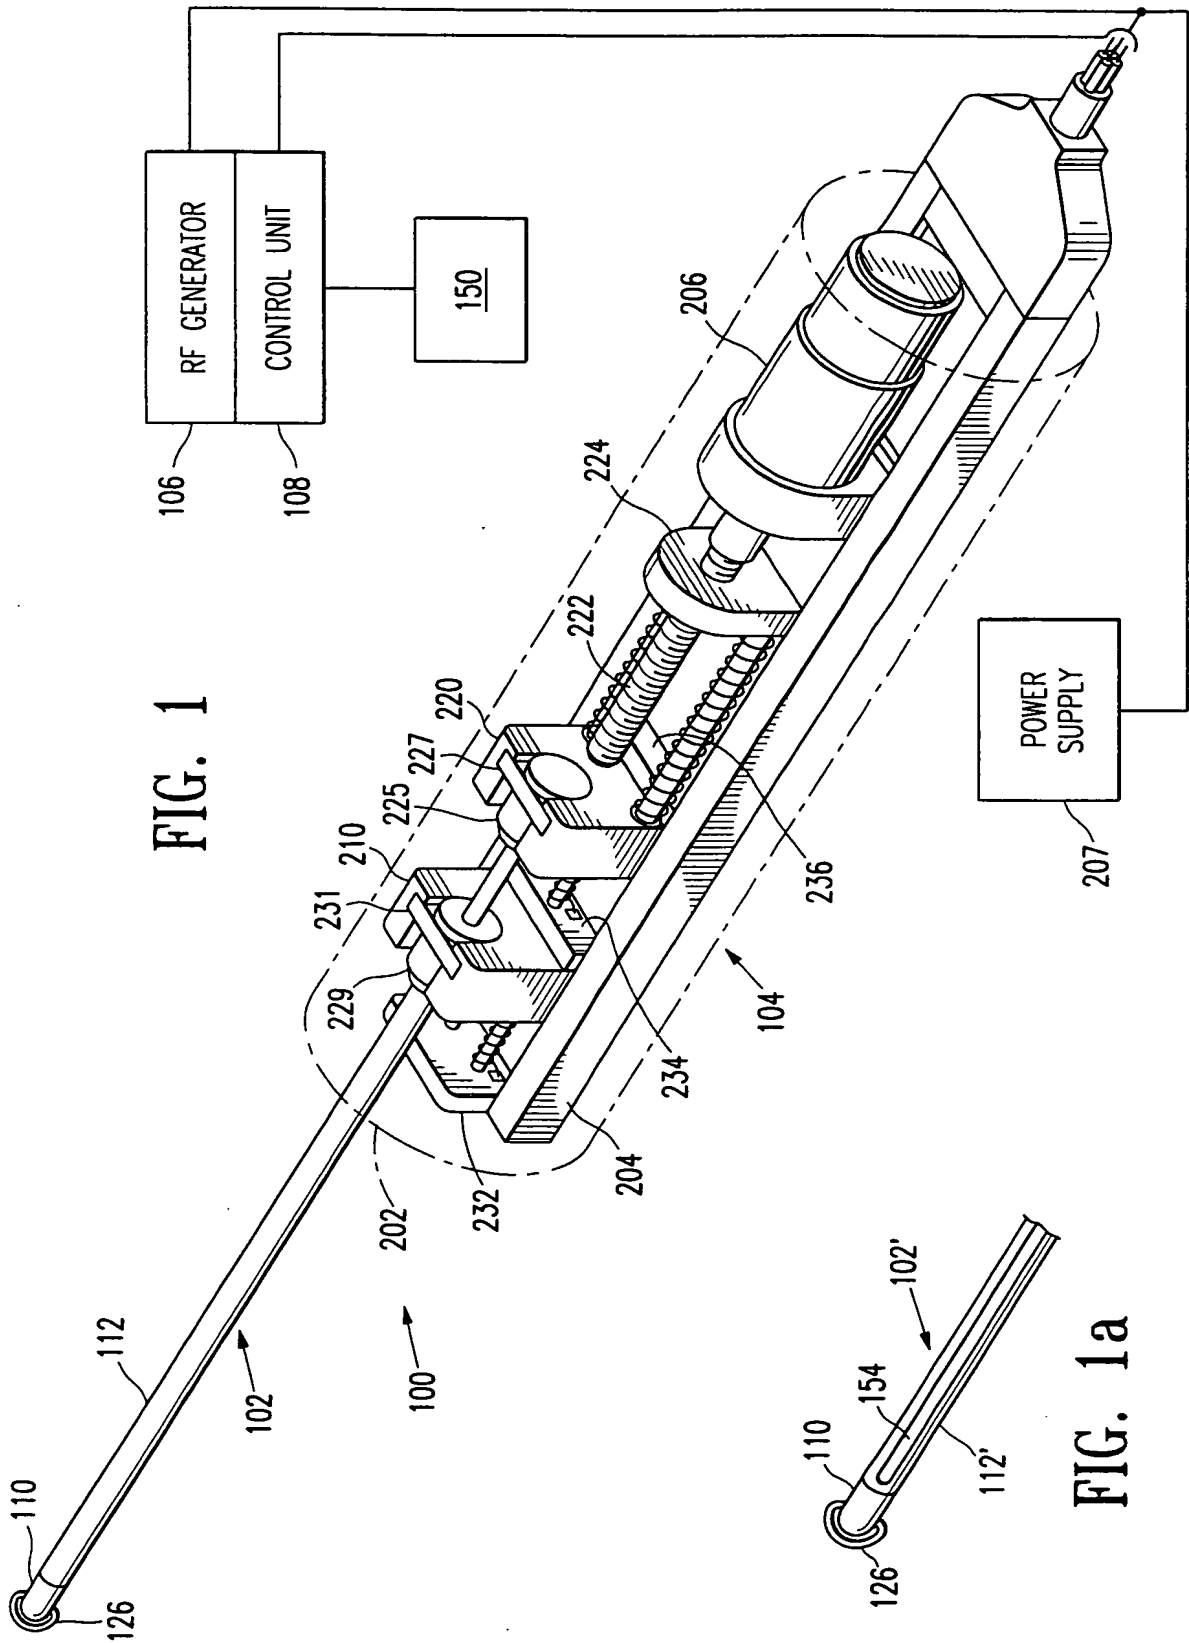


FIG. 1

FIG. 1a

ELECTROSURGICAL BIOPSY DEVICE  
AND METHOD

Inventors: Burbank et al.  
Serial No. 09/819,195  
Sheet 2 of 7

2/7

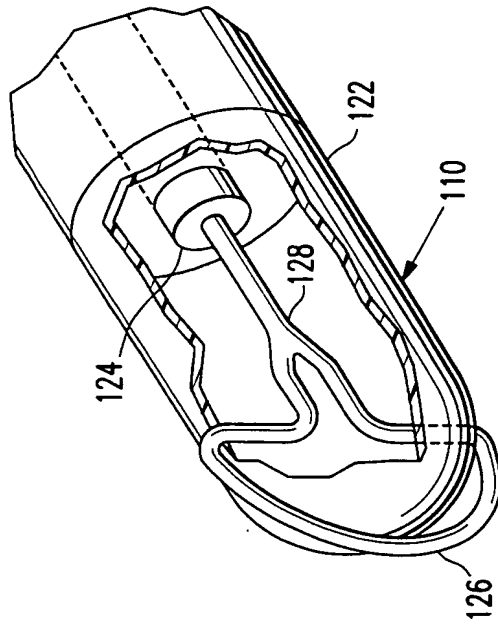


FIG. 3

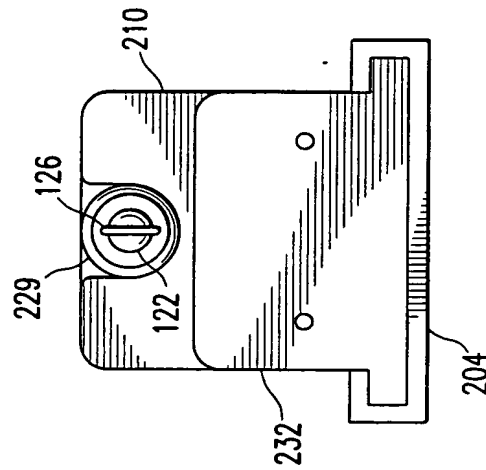


FIG. 2

Inventors: Burbank et al.  
Serial No. 09/819,195  
Sheet 3 of 7

Sheet 3 of 7



# ELECTROSURGICAL BIOPSY DEVICE AND METHOD

Inventors: Burbank et al.

Serial No. 09/819,195

Sheet 4 of 7

4/7

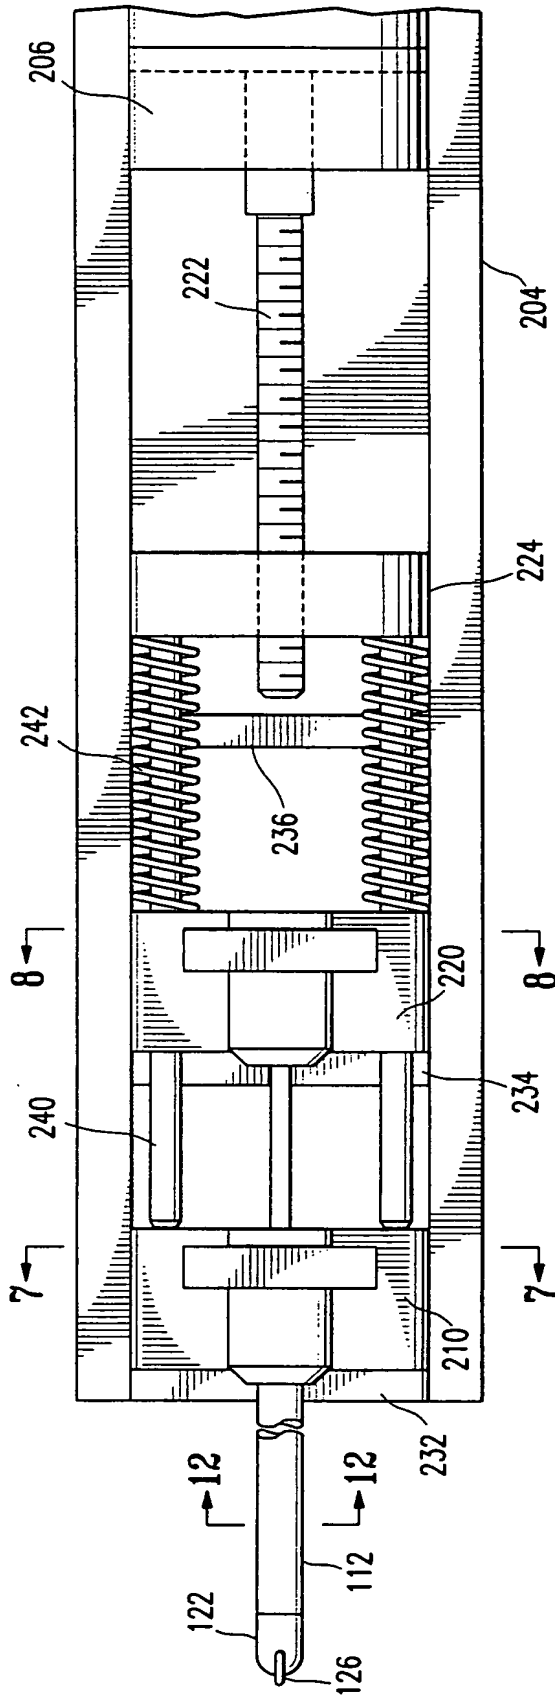


FIG. 6

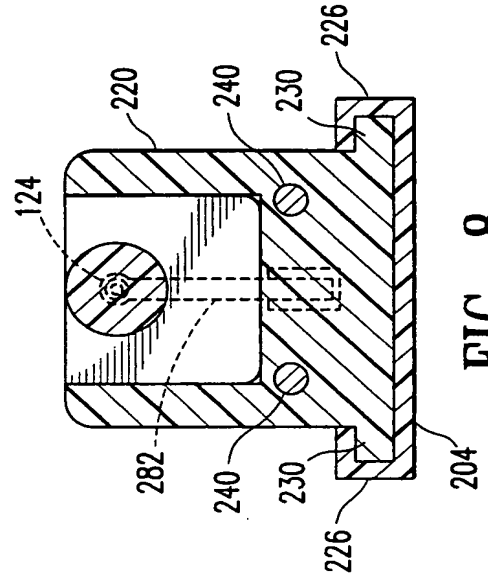


FIG. 8

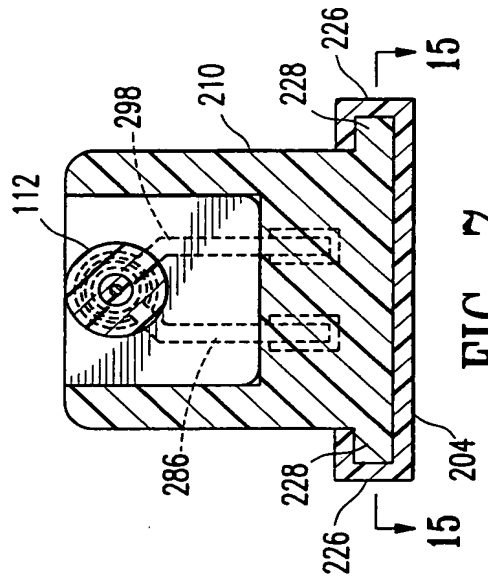


FIG. 7

# ELECTROSURGICAL BIOPSY DEVICE AND METHOD

Inventors: Burbank et al.  
Serial No. 09/819,195  
Sheet 5 of 7

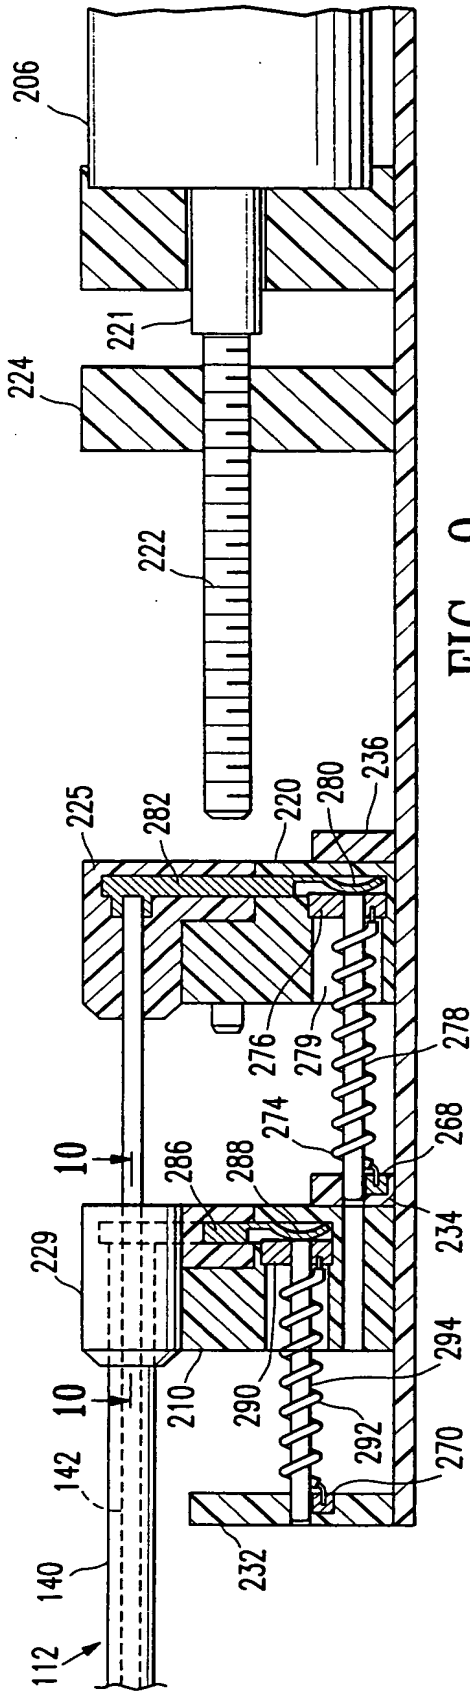


FIG. 9

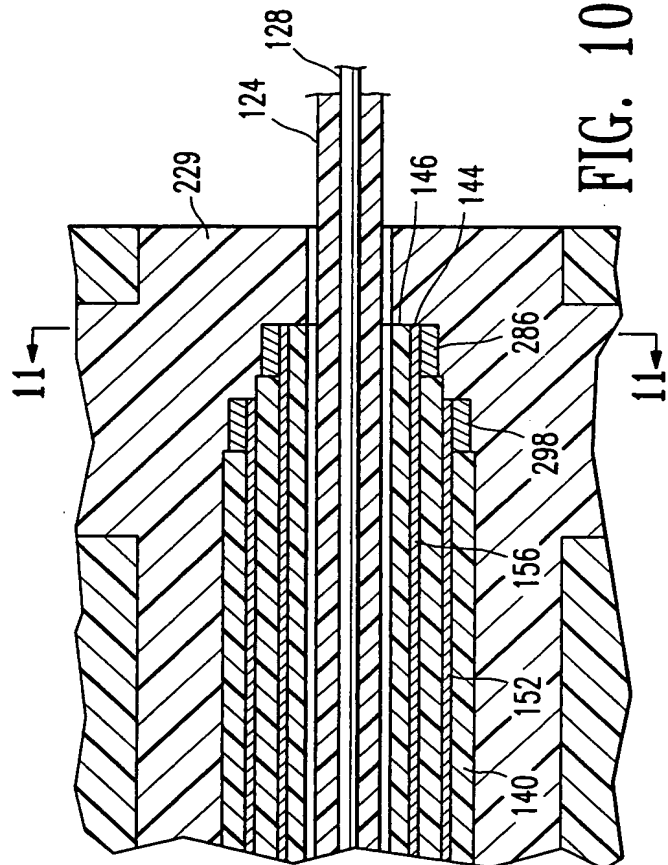


FIG. 10

5/7

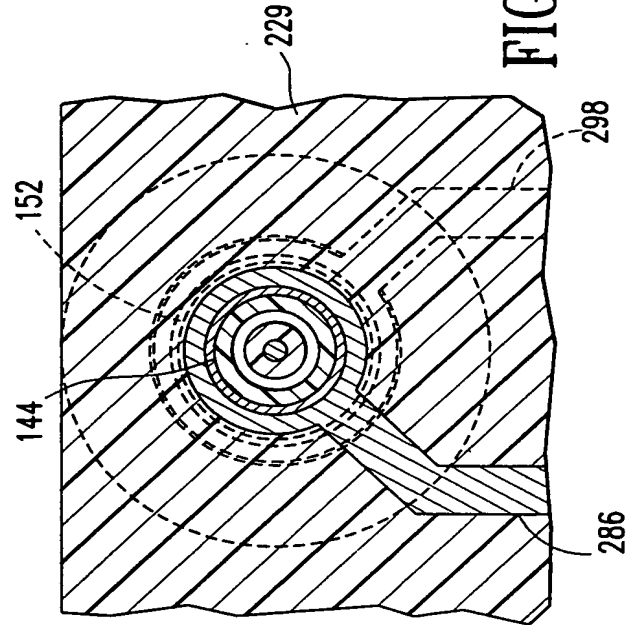


FIG. 11

ELECTROSURGICAL BIOPSY DEVICE  
AND METHOD

Inventors: Burbank et al.

Serial No. 09/819,195

Sheet 6 of 7

6/7

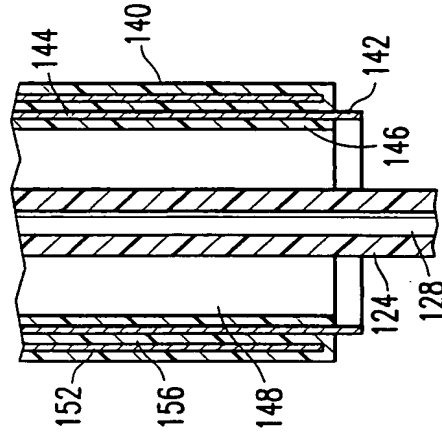


FIG. 14

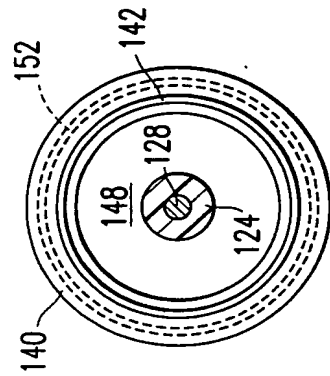


FIG. 13

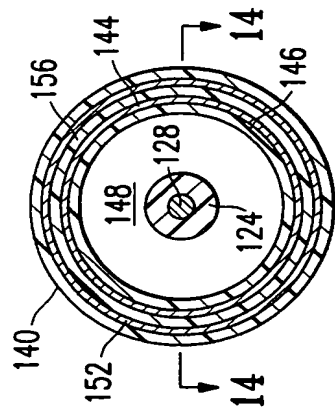


FIG. 12

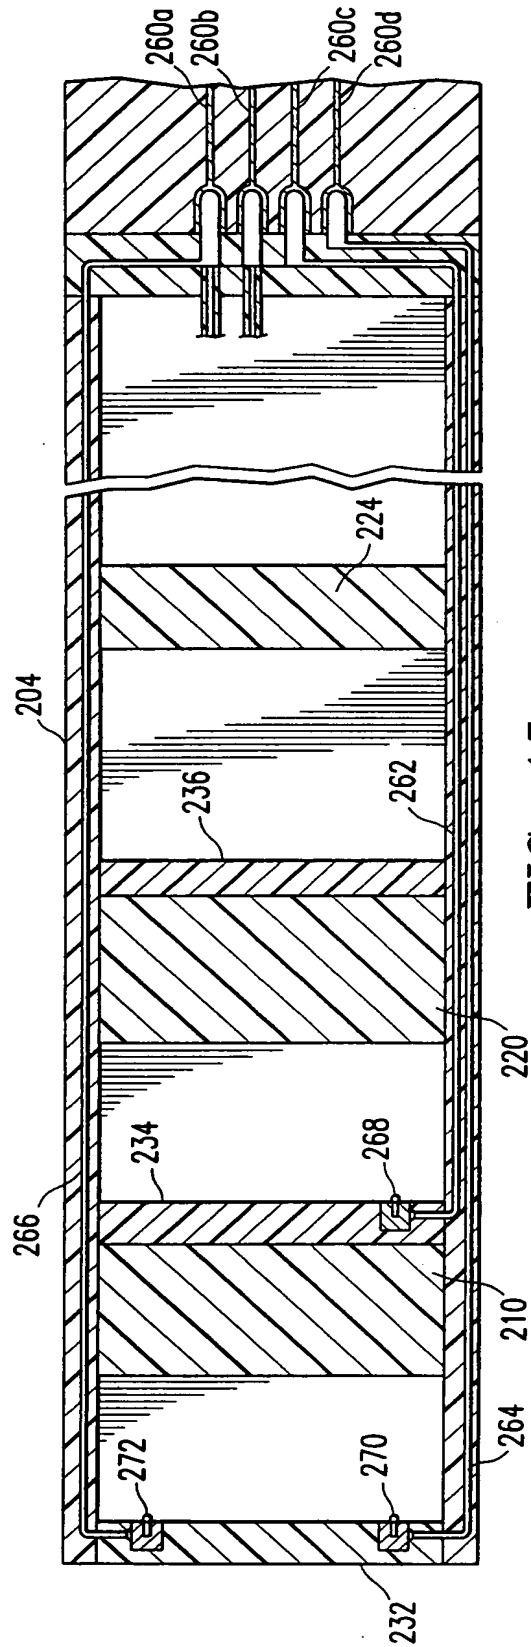


FIG. 15

# ELECTROSURGICAL BIOPSY DEVICE AND METHOD

Inventors: Burbank et al.

Serial No. 09/819,195

Sheet 7 of 7

7/7

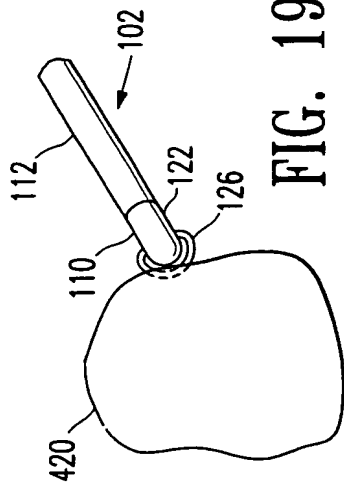


FIG. 19

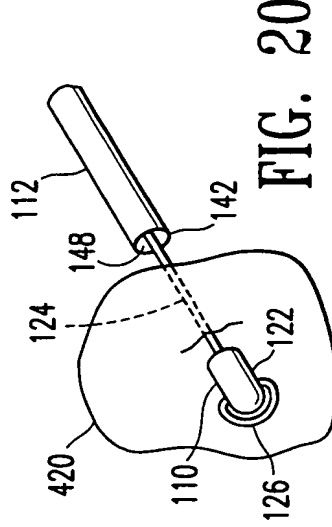


FIG. 20

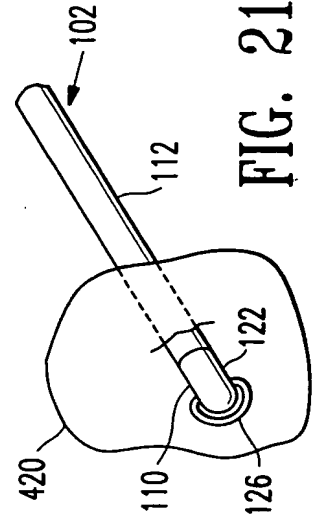


FIG. 21

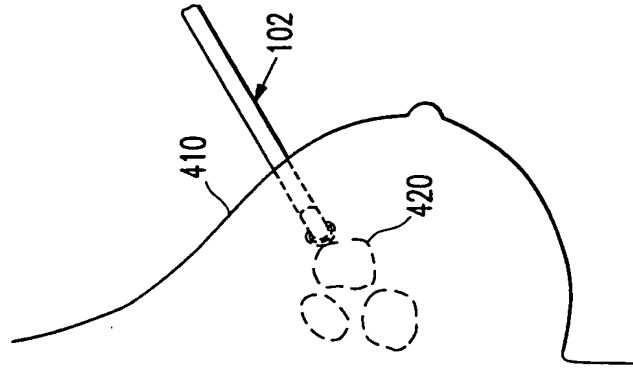


FIG. 18

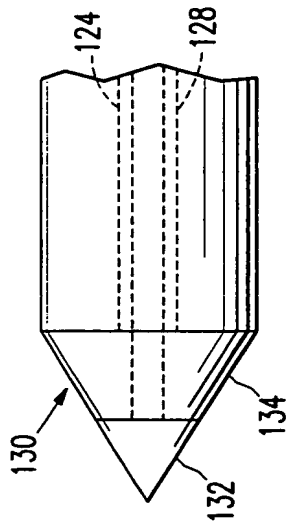


FIG. 16

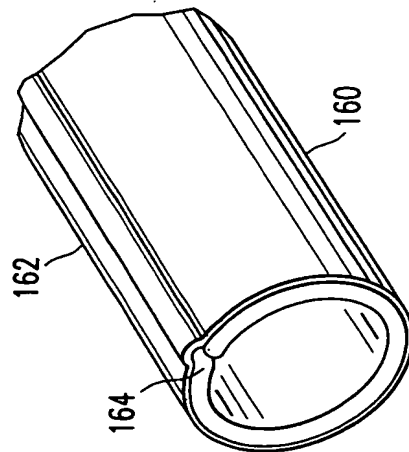


FIG. 17

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☐ **FADED TEXT OR DRAWING**
- ☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☒ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**